

Cat. # RR820L

For Research Use

TAKARA

**TB Green[®] *Premix Ex Taq*[™] II
(Tli RNaseH Plus), Bulk**

Product Manual

v202605w

Table of Contents

I.	Description.....	3
II.	Principle	3
III.	Components	4
IV.	Storage	5
V.	Materials Required but not Provided	5
VI.	Precautions	5
VII.	Protocol.....	6
VIII.	Optimization	15
IX.	Appendix	17
X.	Related Products	19

I. Description

TB Green *Premix Ex Taq II* (Tli RNaseH Plus), Bulk is a reagent specifically designed for intercalator-based real-time PCR using TB Green for detection. The premix is supplied as a 2X concentrate containing TB Green at a concentration appropriate for real-time monitoring, making it easy to prepare reaction mixtures.

The 2X premix also contains Tli RNaseH, a heat-resistant RNase H, which minimizes PCR inhibition due to residual mRNA when using cDNA as the template.

This product contains a modified buffer that offers higher reaction specificity than TB Green *Premix Ex Taq* (Tli RNaseH Plus) (Cat. #RR420A/B). By inhibiting non-specific amplification, which can interfere with quantification, accurate measurement over a wide dynamic range is possible. The combination of this buffer and *TaKaRa Ex Taq®* HS DNA polymerase, a hot-start PCR enzyme that uses an anti-*Taq* antibody, allows highly reproducible and reliable real-time PCR analysis.

Compatible instrument systems include:

- Thermal Cycler Dice™ Real Time System IV (Cat. #TP1000/TP1010/TP1030)
- Thermal Cycler Dice Real Time System III (Cat. #TP950/TP970/TP980/TP990)
- Thermal Cycler Dice Real Time System II (Cat. #TP900/TP960: discontinued)
- Thermal Cycler Dice Real Time System *Lite* (Cat. #TP700/TP760: discontinued)
- Applied Biosystems QuantStudio 3/5 Real-Time PCR System (Thermo Fisher Scientific)
- Applied Biosystems 7500/7500 Fast Real-Time PCR System (Thermo Fisher Scientific)
- Applied Biosystems StepOnePlus Real-Time PCR System (Thermo Fisher Scientific)
- LightCycler/LightCycler 480 System (Roche Diagnostics)
- CFX96 Real-Time PCR Detection System (Bio-Rad)

Note: For the Smart Cycler System/Smart Cycler II System (Cepheid), the use of TB Green *Premix Ex Taq* (Tli RNaseH Plus), Bulk (Cat. #RR420L) is recommended.

II. Principle

This product includes *TaKaRa Ex Taq* HS DNA polymerase for PCR amplification. PCR amplification products may be monitored in real time using TB Green as an intercalator.

1. PCR

PCR is a technique used to amplify a target sequence from a minute amount of DNA. By repeating cycles of denaturation, primer annealing, and elongation, the target gene fragment is amplified by DNA polymerase.

This product uses *TaKaRa Ex Taq* HS DNA Polymerase, a hot-start PCR enzyme that prevents non-specific amplification due to mispriming or primer-dimer formation during reaction mixture preparation or other pre-cycling steps, allowing highly sensitive detection.

2. Fluorescence Detection - Intercalator Method

This method involves the addition of an intercalating agent (TB Green) that fluoresces when bound to double-stranded DNA in the reaction mixture.

Monitoring this fluorescence enables the detection of amplified DNA, quantitative determination of target DNA, and determination of DNA composition by melting curve analysis.

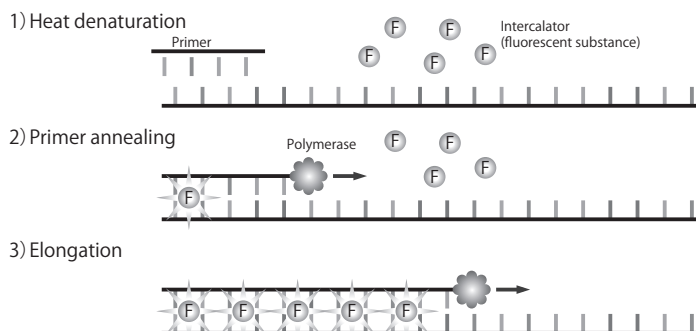


Figure 1. Fluorescent intercalator detection method

III. Components (200 reactions, 50 μ l per reaction)

TB Green <i>Premix Ex Taq</i> II (2X) (Tli RNaseH Plus), Bulk* ¹	5 ml
ROX Reference Dye (50X)* ²	200 μ l

*1 Contains *TAKARA Ex Taq* HS DNA Polymerase, dNTP mixture, Mg²⁺, Tli RNaseH, and TB Green.

*2 ROX Reference Dye is intended for use with instruments that correct for between-well fluorescent signal, such as the real-time PCR instruments by Applied Biosystems.

- ◆ Add the ROX Reference Dye (50X) in a volume equivalent to 1/50 of the PCR reaction mixture when using:
 - Applied Biosystems StepOnePlus Real-Time PCR System (Thermo Fisher Scientific)
- ◆ Add the ROX Reference Dye (50X) in a volume equivalent to 1/250 of the PCR reaction mixture when using:
 - Applied Biosystems QuantStudio 3/5 Real-Time PCR System
 - Applied Biosystems 7500/7500 Fast Real-Time PCR System (Both models are made by Thermo Fisher Scientific.)
- ◆ Do not use this reference dye with:
 - Thermal Cycler Dice Real Time System series*³
 - LightCycler/LightCycler 480 System (Roche Diagnostics)
 - CFX96 Real-Time PCR Detection System (Bio-Rad)

*³ Not available in all geographic locations. Check for availability in your area.

IV. Storage

Store at 4°C (stable for up to 6 months.)

Always protect from light and avoid contamination.

For long-term storage, store at -20°C. Store thawed or opened product at 4°C and use within 6 months.

V. Materials Required but not Provided

- Gene amplification system for real-time PCR (authorized instruments)
- Real-time PCR reaction tubes or plates designed specifically for the qPCR instrument used
- PCR primers
For guidelines on real-time PCR primer design, refer to Section IX-1.
- Sterile purified water
- Micropipettes and tips (sterile filter tips)

VI. Precautions

Read these precautions before use and follow them when using this product.

1. Prior to use, make sure the reagent is evenly mixed by gently inverting several times without creating bubbles. Uneven reagent mixture will result in inadequate reactivity.
 - Do not mix by vortexing.
 - When stored at -20°C, TB Green *Premix Ex Taq* II (2X) (Tli RNaseH Plus), Bulk may develop a white to pale yellow precipitate. Gently hand-warm and allow to stand protected from light at room temperature briefly, then invert several times to dissolve the precipitate completely.
 - The presence of precipitate is indicative of uneven reagent composition; make sure the reagent is evenly mixed before use.
2. Place reagents on ice immediately after thawing, and keep them on ice while preparing the reaction mixture.
3. This product contains TB Green. Avoid exposure to bright light while preparing the reaction mixture.
4. While preparing or dispensing reaction mixtures, use sterile, disposable tips to avoid contamination between samples.

VII. Protocol

Note: Please follow the procedures in the manual provided with each respective instrument.

[For the Applied Biosystems QuantStudio 3/5 Real-Time PCR System, 7500/7500 Fast Real-Time PCR Systems, and StepOnePlus Real-Time PCR System]

A. Prepare the PCR mixture shown below.

- When using the StepOnePlus Real-Time PCR System, add ROX Reference Dye (50X) in a volume equivalent to 1/50 of the PCR reaction mixture. To account for pipetting error, make a master mix with at least 10% more than the total volume needed for the total number of reactions.

<Per reaction>

Reagent	Volume	Final conc.
TB Green <i>Premix Ex Taq</i> II (2X) (Tli RNaseH Plus), Bulk	10 μ l	1X
PCR Forward Primer (10 μ M)	0.8 μ l	0.4 μ M*1
PCR Reverse Primer (10 μ M)	0.8 μ l	0.4 μ M*1
ROX Reference Dye (50X)	0.4 μ l	1X
Template (<100 ng)*2	2 μ l	
Sterile purified water	6 μ l	
Total	20 μl	

- When using the Applied Biosystems QuantStudio 3/5 or 7500/7500 Fast Real-Time PCR Systems, add ROX Reference Dye (50X) in a volume equivalent to 1/250 of the PCR reaction mixture. To account for pipetting error, make a master mix with at least 10% more than the total volume needed for the total number of reactions.

<Per reaction>

Reagent	Volume	Volume	Final conc.
TB Green <i>Premix Ex Taq</i> II (2X) (Tli RNaseH Plus), Bulk	10 μ l	25 μ l	1X
PCR Forward Primer (10 μ M)	0.8 μ l	2 μ l	0.4 μ M*1
PCR Reverse Primer (10 μ M)	0.8 μ l	2 μ l	0.4 μ M*1
ROX Reference Dye (50X)	0.08 μ l	0.2 μ l	0.2X
Template*2	2 μ l	4 μ l	
Sterile purified water	6.32 μ l	16.8 μ l	
Total	20 μl*3	50 μl*3	

- *1 A final primer concentration of 0.4 μ M is likely to yield good results. However, if there is insufficient reactivity, use a primer concentration between 0.2 and 1.0 μ M.
- *2 The optimal quantity varies depending on the number of target copies present in the template solution. Make serial dilutions to determine the appropriate template amount and use no more than 100 ng of DNA template per 20 μ l. Furthermore, if cDNA is used as the template in the RT reaction mixture, the volume of the RT reaction mixture should not exceed 10% of the PCR mixture.
- *3 Prepare in accordance with the recommended volume for each instrument.

B. Start the reaction.

The recommended two-step PCR standard protocol is described below. Try this protocol first and optimize PCR conditions as necessary. Perform 3-step PCR when using primers with low T_m values or when two-step PCR is not feasible. To further optimize PCR conditions, please see section VIII. Optimization.

1) Applied Biosystems QuantStudio 3/5 Real-Time PCR System

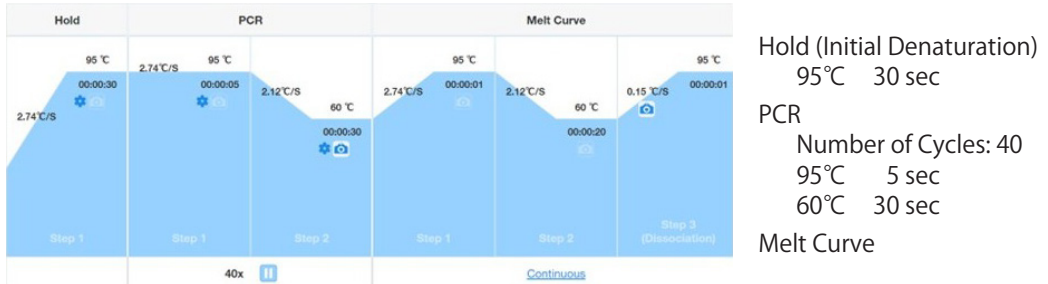


Figure 2. Two-step PCR standard protocol

2) Applied Biosystems 7500 and StepOnePlus Real-Time PCR System

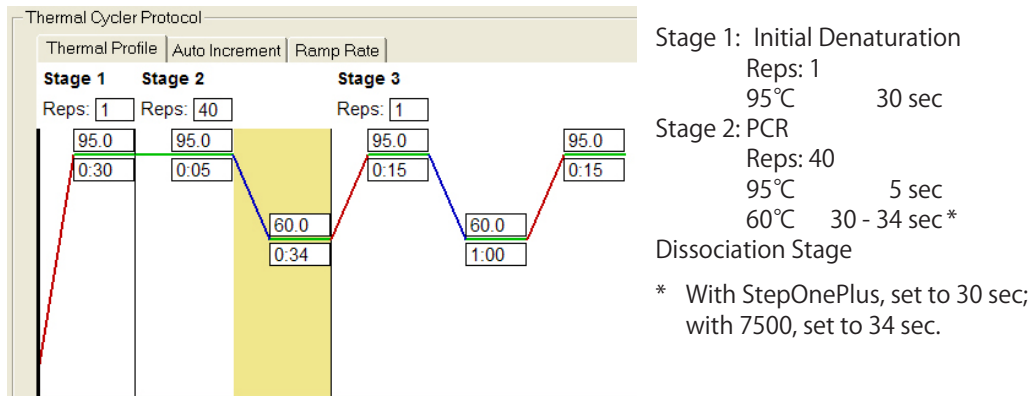


Figure 3. Two-step PCR standard protocol

3) Applied Biosystems 7500 Fast Real-Time PCR System

Two-step PCR standard protocol

Holding Stage

Number of Cycle: 1

95°C 30 sec

Cycling Stage

Number of Cycles: 40

95°C 3 sec

60°C 30 sec

Melt Curve Stage

Note:

TAKARA Ex Taq HS DNA Polymerase is a hot-start PCR enzyme with an anti-*Taq* antibody that inhibits polymerase activity. The initial denaturation step prior to PCR should be 95°C for 30 sec. Longer heat treatment may decrease enzyme activity and affect amplification efficiency and quantification.

- C. After the reaction is complete, check the amplification and melting curves and plot a standard curve if quantification will be performed.

Refer to the instrument's instruction manual for specific analysis methods.

[For the LightCycler/LightCycler 480 System]

- A. Prepare the PCR mixture shown below. To account for pipetting error, make a master mix with at least 10% more than the total volume needed for the total number of reactions.

<Per reaction>


Reagent	Volume	Final conc.
TB Green <i>Premix Ex Taq</i> II (2X) (Tli RNaseH Plus), Bulk	10 μ l	1X
PCR Forward Primer (10 μ M)	0.8 μ l	0.4 μ M*1
PCR Reverse Primer (10 μ M)	0.8 μ l	0.4 μ M*1
Template (<100 ng)*2	2 μ l	
Sterile purified water	6.4 μ l	
Total	20 μl	

- *1 A final primer concentration of 0.4 μ M is likely to yield good results. However, if there is insufficient reactivity, use a primer concentration between 0.2 and 1.0 μ M.
- *2 The optimal quantity varies depending on the number of target copies present in the template solution. Make serial dilutions to determine the appropriate template amount and use no more than 100 ng of DNA template per 20 μ l. Furthermore, if cDNA is used as the template in the RT reaction mixture, the volume of the RT reaction mixture should not exceed 10% of the PCR reaction mixture.

- B. Start the reaction.

The two-step PCR standard protocol is recommended for PCR. Try this protocol first and optimize PCR conditions as necessary. Perform 3-step PCR when using primers with low Tm values or when two-step PCR is not feasible. To further optimize PCR conditions, please see section VIII. Optimization.

<LightCycler>

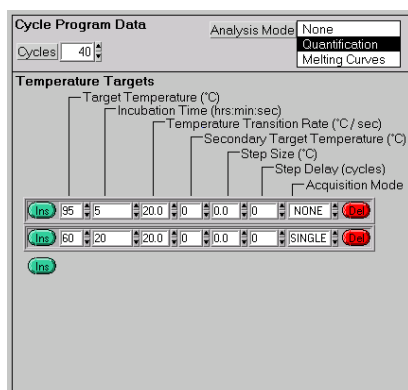

- Stage 1: Initial Denaturation
95°C 30 sec 20°C/sec
1 cycle
- Stage 2: PCR
95°C 5 sec 20°C/sec
60°C 20 sec 20°C/sec
40 cycles
- Stage 3: Melt Curve Analysis
95°C 0 sec 20°C/sec
65°C 15 sec 20°C/sec
95°C 0 sec 0.1°C/sec

Figure 4. Two-step PCR standard protocol

<LightCycler 480 System>

The screenshot shows the 'Programs' section with the following data:

Program Name	Cycles	Analysis Mode
Denaturation	1	None
PCR	40	Quantification
Melting	1	Melting Curves
Cooling	1	None

The 'PCR Temperature Targets' section shows the following data:

Target (°C)	Acquisition Mode	Hold (hh:mm:ss)	Ramp Rate (°C/s)	Acquisitions (per °C)	Sec Target (°C)	Step Size (°C)	Step Delay (cycles)
95	None	00:00:05	4.4	0	0	0	0
60	Single	00:00:30	2.2	0	0	0	0

Figure 5. Two-step PCR standard protocol

Initial Denaturation

95°C 30 sec (Ramp Rate 4.4°C/sec)
1 cycle

PCR

Analysis Mode: Quantification

95°C 5 sec (Ramp Rate 4.4°C/sec)
60°C 30 sec (Ramp Rate 2.2°C/sec, Acquisition Mode: Single)
40 cycles

Melting

Analysis Mode: Melting Curves

95°C 5 sec (Ramp Rate 4.4°C/sec)
60°C 1 min (Ramp Rate 2.2°C/sec)
95°C (Ramp Rate 0.11°C/sec, Acquisition Mode: Continuous, Acquisitions: 5 per°C)
1 cycle

Cooling

50°C 30 sec (Ramp Rate 2.2°C/sec)
1 cycle

Note:

TAKARA Ex Taq HS DNA Polymerase is a hot-start PCR enzyme with an anti-*Taq* antibody that inhibits polymerase activity. The initial denaturation step prior to PCR should be 95°C for 30 sec. Longer heat treatment may decrease enzyme activity and affect amplification efficiency and quantification.

- C. After the reaction is complete, check the amplification and melting curves and plot a standard curve if quantification will be performed.
Refer to the instrument's instruction manual for specific analysis methods.

[For the CFX96 Real-Time PCR Detection System]

- A. Prepare the PCR mixture shown below. To account for pipetting error, make a master mix with at least 10% more than the total volume needed for the total number of reactions.


<Per reaction>

Reagent	Volume	Final conc.
TB Green <i>Premix Ex Taq</i> II (2X) (Tli RNaseH Plus), Bulk	12.5 μ l	1X
PCR Forward Primer (10 μ M)	1 μ l	0.4 μ M*1
PCR Reverse Primer (10 μ M)	1 μ l	0.4 μ M*1
Template (<100 ng)*2	2 μ l	
Sterile purified water	8.5 μ l	
Total	25 μ l	

- *1 A final primer concentration of 0.4 μ M is likely to yield good results. However, if there is insufficient reactivity, use a primer concentration between 0.2 and 1.0 μ M.
- *2 The optimal quantity varies depending on the number of target copies present in the template solution. Make serial dilutions to determine the appropriate template amount and use no more than 100 ng of DNA template per 25 μ l. Furthermore, if cDNA is used as the template in the RT reaction mixture, the volume of the RT reaction mixture should not exceed 10% of the PCR mixture.

B. Start the reaction.

The two-step PCR standard protocol is recommended for PCR; try this protocol first and optimize PCR conditions as necessary. Perform 3-step PCR when using primers with low T_m values or when two-step PCR is not feasible. For guidelines on optimizing PCR conditions, please refer to Section VIII.

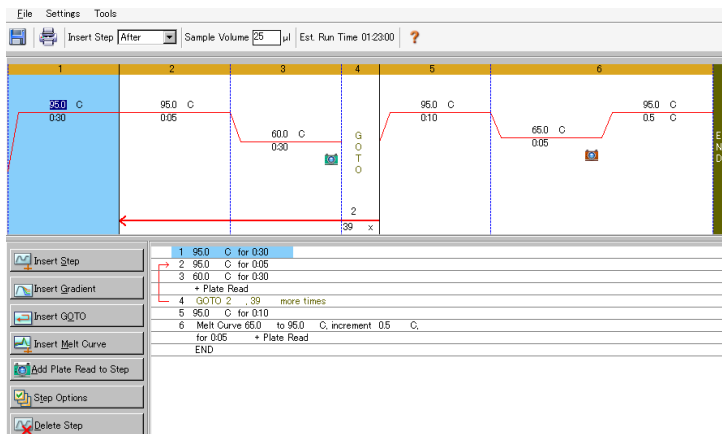Sample volume: 25 μ lStep 1: Initial Denaturation
95°C 30 secStep 2: PCR
GOTO: 39 (40 cycles)
95°C 5 sec
60°C 30 sec

Step 3: Melt Curve

Figure 6. Two-step PCR standard protocol

Note:

TaKaRa Ex Taq HS DNA Polymerase is a hot-start PCR enzyme with an anti-*Taq* antibody that inhibits polymerase activity. The initial denaturation step prior to PCR should be 95°C for 30 sec. Longer heat treatment may decrease enzyme activity and affect amplification efficiency and quantification.

C. After the reaction is complete, check the amplification and melting curves and plot a standard curve if quantification will be performed.

Refer to the instrument's instruction manual for specific analysis methods.

[For the Thermal Cycler Dice Real Time System series]

- A. Prepare the PCR mixture shown below. To account for pipetting error, make a master mix with at least 10% more than the total volume needed for the total number of reactions.

<Per reaction>

Reagent	Volume	Final conc.
TB Green <i>Premix Ex Taq</i> II (2X) (Tli RNaseH Plus), Bulk	12.5 μ l	1X
PCR Forward Primer (10 μ M)	1.0 μ l	0.4 μ M* ¹
PCR Reverse Primer (10 μ M)	1.0 μ l	0.4 μ M* ¹
Template (<100 ng)* ²	2.0 μ l	
Sterile purified water	8.5 μ l	
Total	25 μ l* ³	

- *1 A final primer concentration of 0.4 μ M is likely to yield good results. However, if there is insufficient reactivity, use a primer concentration between 0.2 and 1.0 μ M.
- *2 The optimal quantity varies depending on the number of target copies present in the template solution. Make serial dilutions to determine the appropriate template amount and use no more than 100 ng of DNA template per 25 μ l. Furthermore, if cDNA is used as the template in the RT reaction mixture, the volume of the RT reaction mixture should not exceed 10% of the PCR reaction mixture.
- *3 The recommended volume is 25 μ l.

B. Start the reaction.

The two-step PCR standard protocol is recommended; try this protocol first and optimize PCR conditions as necessary. Perform a 3-step PCR when using primers with low T_m values or when two-step PCR is not feasible. To optimize PCR conditions, please refer to Section VIII.

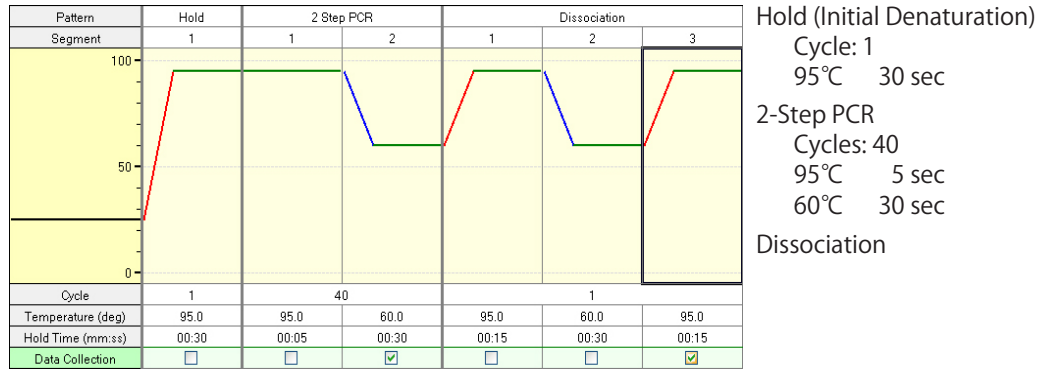


Figure 7. Two-step PCR standard protocol

Note:

TaKaRa Ex Taq HS DNA Polymerase is a hot-start PCR enzyme with an anti-*Taq* antibody that inhibits polymerase activity. The initial denaturation step prior to PCR should be 95°C for 30 sec. Longer heat treatment may decrease enzyme activity and affect amplification efficiency and quantification.

C. After the reaction is complete, check the amplification and melting curves and plot a standard curve if quantification will be performed.

Refer to the instrument's instruction manual for specific analysis methods.

VIII. Optimization


If the recommended conditions (two-step PCR standard protocol) do not provide sufficient reactivity, follow the procedures below to optimize primer concentration and PCR conditions. Depending on the reaction system, switching to a different real-time PCR reagent from the Perfect Real Time series (Cat. #RR420A/B/L, RR091A/B) may greatly improve the results.

Select PCR conditions based on comprehensive analysis of reaction specificity and amplification efficiency. Using conditions that balance these two aspects will allow accurate measurement over a wide range of concentrations.

- System with a high reaction specificity
 - Using a negative, no-template control, non-specific amplification (e.g., primer dimers) does not occur.
 - Non-specific amplification products (those other than the target product) are not generated.
- System with a high amplification efficiency
 - Amplification product is detected at earlier cycles (lower Ct value).
 - PCR amplification efficiency is high (near the theoretical value of 100%).

1. Evaluation of primer concentration


The relationship between primer concentration, reaction specificity, and amplification efficiency is illustrated below. Reducing primer concentration raises reaction specificity, whereas increasing the primer concentration raises amplification efficiency.



2. Evaluation of PCR conditions


- To improve reaction specificity

Raising the annealing temperature may improve reaction specificity. Perform optimization while checking amplification efficiency.

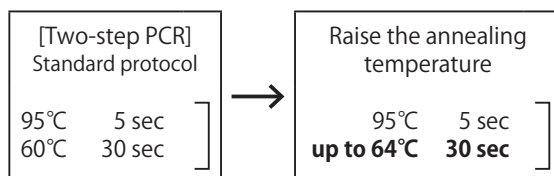

- To improve amplification efficiency

Increasing the elongation time or switching to 3-step PCR may improve amplification efficiency. Perform optimization using the steps below.

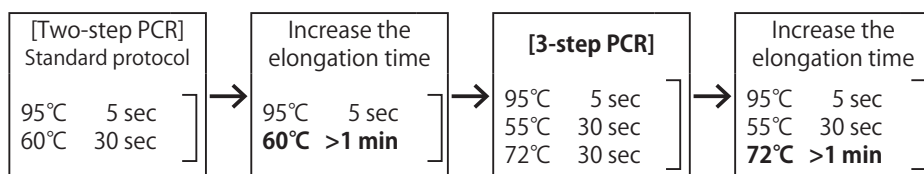

- Initial denaturation


Generally, 95°C for 30 sec is sufficient for initial denaturation, even for difficult to denature templates such as circular plasmids and genomic DNA. This procedure may be extended to 1 - 2 min at 95°C depending on the template. However, prolonging this step may inactivate the enzyme. Therefore, it is recommended to avoid initial denaturation steps >2 min.

3. Relationship between reagent and reactivity

Takara Bio supplies several different reagents for intercalator-based real-time PCR analysis using TB Green. The relationship between reaction specificity and amplification efficiency for these reagents is described below.

TB Green *Premix Ex Taq* (Tli RNaseH Plus) (Cat. #RR420A/B/L) provides high amplification efficiency. TB Green *Premix Ex Taq* II (Tli RNaseH Plus) (Cat. #RR820A/B/L) and TB Green *Premix DimerEraser*™ (Perfect Real Time) (Cat. #RR091A/B) have greater specificity.

(Reagent)

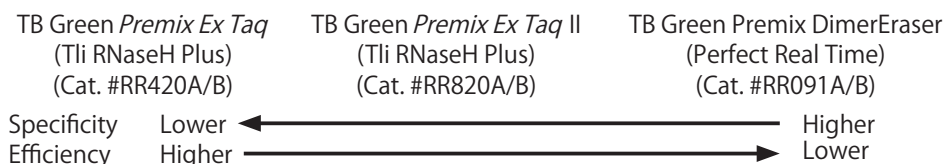

IX. Appendix**1. Primer design**

Designing primers with a good reactivity is critical to successful real-time PCR. Follow the guidelines below to design primers that yield high amplification efficiency without non-specific amplification.

RT-PCR primers designed and synthesized using these guidelines are compatible with the two-step PCR standard protocol (Section VII.).

■ Amplification product

Amplification size	The optimal size is 80 - 150 bp (amplification up to 300 bp is possible).
--------------------	---

■ Primer

Length	17 - 25 mer
GC content	40 - 60% (preferably 45 - 55%)
Tm	Make sure the Tm values for the forward primer and the reverse primer do not differ greatly. Use software to determine Tm values. OLIGO*1 : 63 - 68°C Primer3 : 60 - 65°C
Sequence	Make sure there are no overall base sequence biases. Avoid having any GC-rich or AT-rich regions in the sequence (particularly at the 3' end). Avoid having consecutive T/C pairings (polypyrimidine). Avoid having consecutive A/G pairings (polypurine).
3' end sequence	Avoid having GC-rich or AT-rich regions at the 3' end. It is preferable to have a G or C as the terminal base at the 3' end. Avoid a primer design with T as the terminal base at the 3' end.
Complementation	Avoid having any complementary sequences of three bases or more within a primer and between primers. Avoid having any complementary sequences of two bases or more at a primer's 3' end.
Specificity	Verify primer specificity with a BLAST search.*2

*1 OLIGO Primer Analysis Software (Molecular Biology Insights, Inc.)

*2 <https://blast.ncbi.nlm.nih.gov/Blast.cgi>

2. Preparing templates for real-time RT-PCR

When preparing cDNA templates for real-time RT-PCR, the following products are recommended

- PrimeScript™ RT reagent Kit (Perfect Real Time) (Cat. #RR037A/B)
- PrimeScript RT Master Mix (Perfect Real Time) (Cat. #RR036A/B)
- PrimeScript RT Reagent Kit with gDNA Eraser (Perfect Real Time) (Cat. #RR047A/B)

When used in combination with this kit, these products provide reliable results. Refer to the product's user manual for RT reaction conditions.

- A. Prepare PCR mixtures according to the following procedure.
(When using Thermal Cycler Dice Real Time System II: discontinued)

Prepare the following components in volumes slightly more than what is needed for the required number of tubes and dispense 22.5 - 24 μ l.

<Per reaction>

Reagent	Volume	Final conc.
TB Green <i>Premix Ex Taq</i> II (2X) (Tli RNaseH Plus), Bulk	12.5 μ l	1X
PCR Forward Primer (10 μ M)	1.0 μ l	0.4 μ M
PCR Reverse Primer (10 μ M)	1.0 μ l	0.4 μ M
Sterile purified water	x μ l	
Total	22.5 - 24 μl	

- B. Add 1.0 - 2.5 μ l of the RT reaction mixture to each of the microtubes containing aliquots of the PCR reaction mixture.

Note: Add no more than 2.5 μ l of the RT reaction mixture to the PCR reaction mixture.

[Experimental example]

Human TBP mRNA was detected by real-time RT-PCR. cDNA equivalent to 1 pg - 100 ng of total RNA was used as the template, with sterile purified water as the negative control.

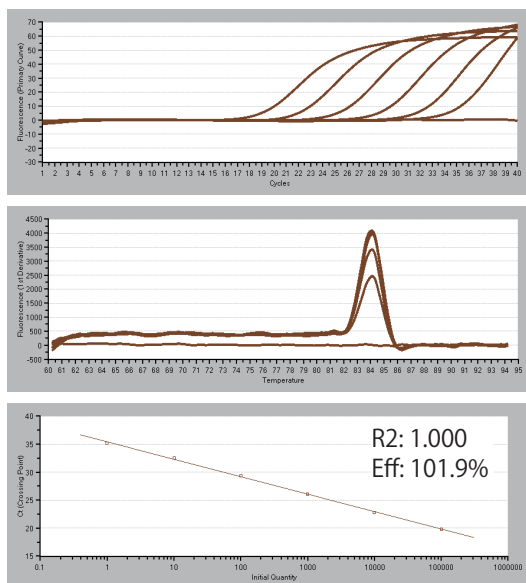


Figure 8. Detection of human TBP mRNA by real-time RT-PCR

X. Related Products

TB Green® *Premix Ex Taq*™ II (Tli RNaseH Plus) (Cat. #RR820S/A/B)*
TB Green® *Premix Ex Taq*™ II (Tli RNaseH Plus), ROX plus (Cat. #RR82LR/WR)*
TB Green® Fast qPCR Mix (Cat. #RR430A/B)
TB Green® *Premix Ex Taq*™ (Tli RNaseH Plus) (Cat. #RR420S/A/B)*
TB Green® *Premix Ex Taq*™ (Tli RNaseH Plus), Bulk (Cat. #RR420L/W)*
TB Green® *Premix Ex Taq*™ (Tli RNaseH Plus), ROX plus (Cat. #RR42LR/WR)*
TB Green® Premix DimerEraser™ (Perfect Real Time) (Cat. #RR091A/B)*
TB Green® *Premix Ex Taq*™ GC (Perfect Real Time) (Cat. #RR071A/B)*
PrimeScript™ RT reagent Kit (Perfect Real Time) (Cat. #RR037A/B)
PrimeScript™ RT Master Mix (Perfect Real Time) (Cat. #RR036A/B)
PrimeScript™ RT Reagent Kit with gDNA Eraser (Perfect Real Time) (Cat. #RR047A/B)

Thermal Cycler Dice™ Real Time System IV (Cat. #TP1000/TP1010/TP1030)*
Thermal Cycler Dice™ Real Time System III (Cat. #TP950/TP970/TP980/TP990)*

* Not available in all geographic locations. Check for availability in your area.

TB Green and *TakaRa Ex Taq* are registered trademarks of Takara Bio Inc.
Premix Ex Taq, Thermal Cycler Dice, DimerEraser, and PrimeScript are trademarks of Takara Bio Inc.

NOTE: This product is for research use only. It is not intended for use in therapeutic or diagnostic procedures for humans or animals. Also, do not use this product as food, cosmetic, or household item, etc.

Takara products may not be resold or transferred, modified for resale or transfer, or used to manufacture commercial products without written approval from Takara Bio Inc.

If you require licenses for other use, please contact us from our website at www.takarabio.com.

Your use of this product is also subject to compliance with any applicable licensing requirements described on the product web page. It is your responsibility to review, understand and adhere to any restrictions imposed by such statements.

All trademarks are the property of their respective owners. Certain trademarks may not be registered in all jurisdictions.